



Below is the proper set up on the surgical table when using a HotDog Warming Mattress + Return Electrode with and without the use of an inflatable transfer device.

Table Stack


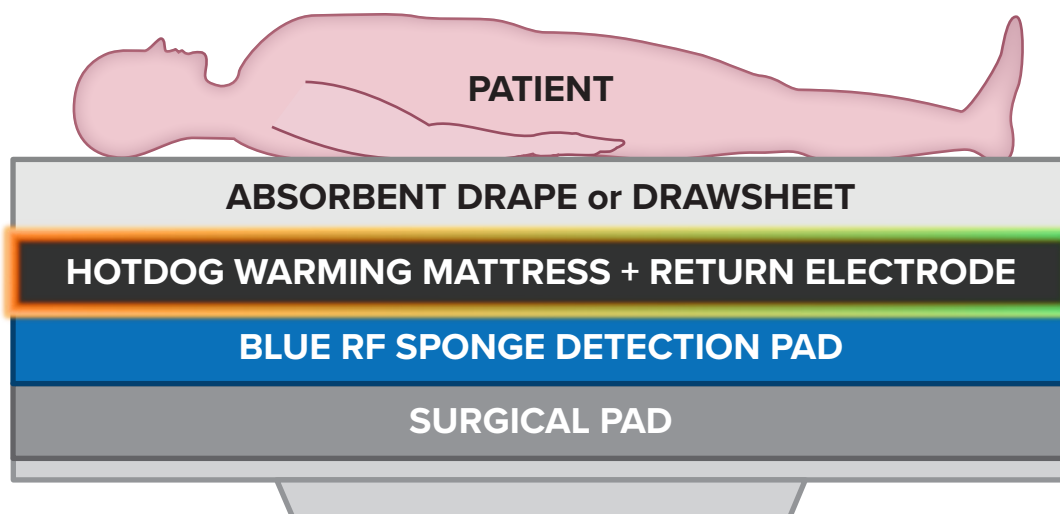


Table Stack with Transfer Device

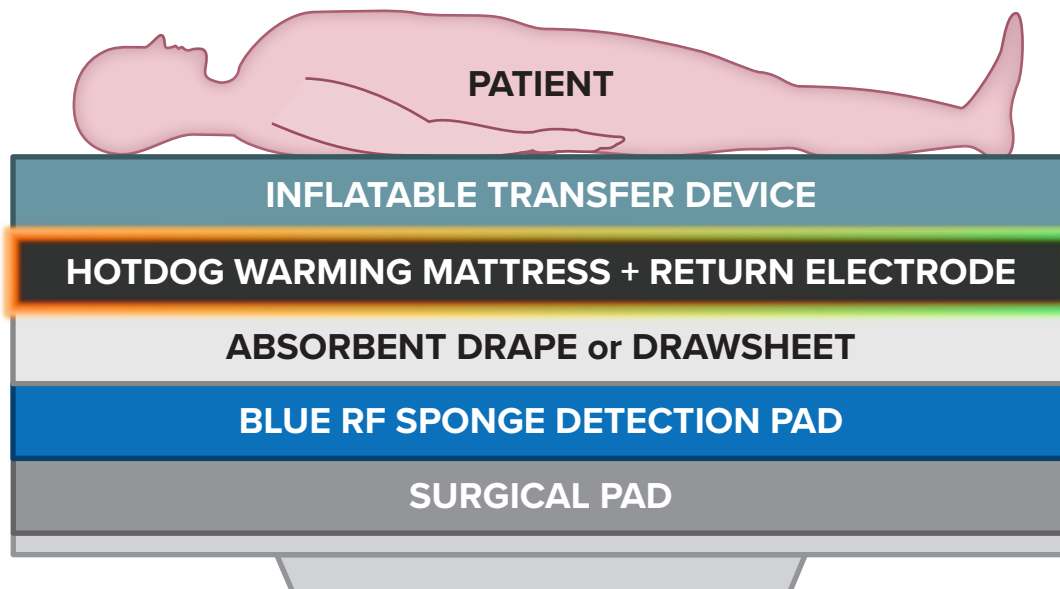

Drawings not to scale.